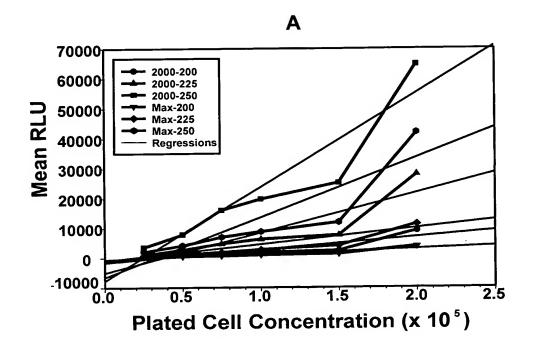


Fig. 1



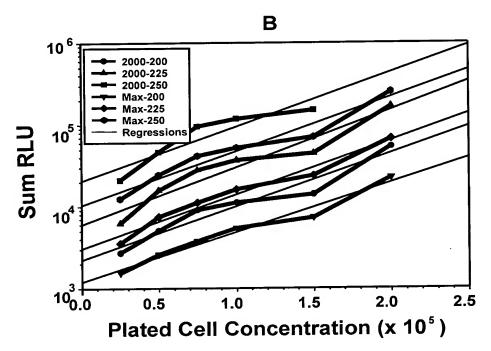


Fig. 2

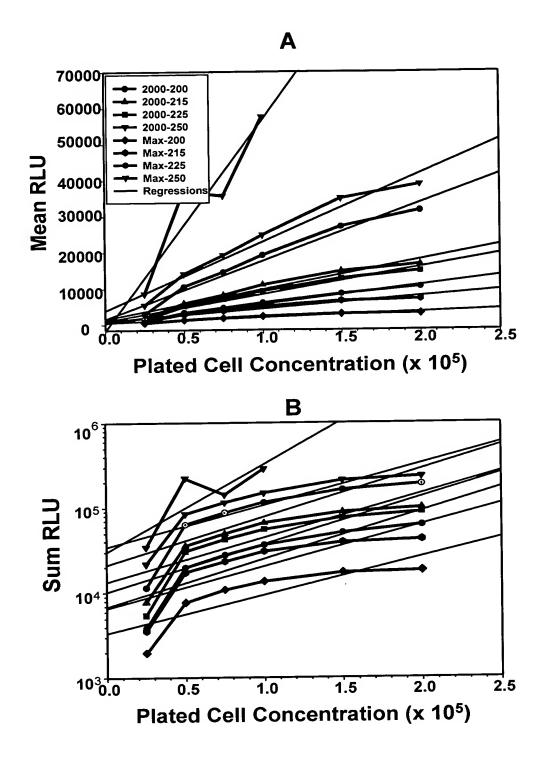


Fig. 3

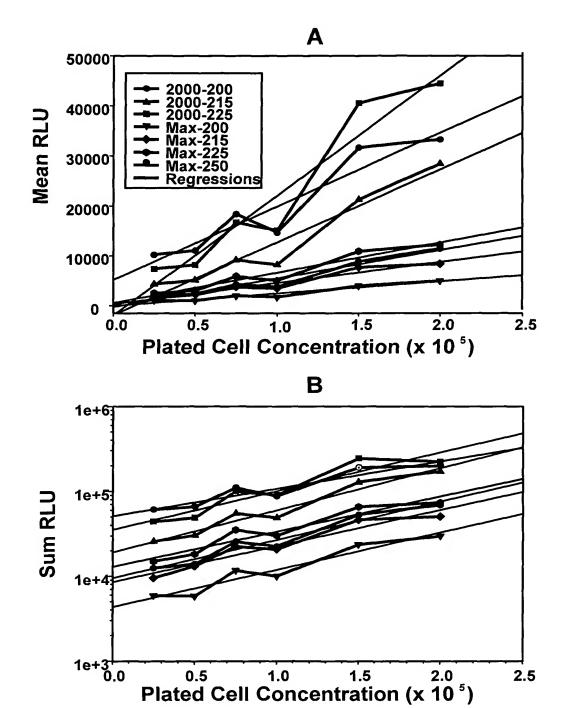


Fig. 4

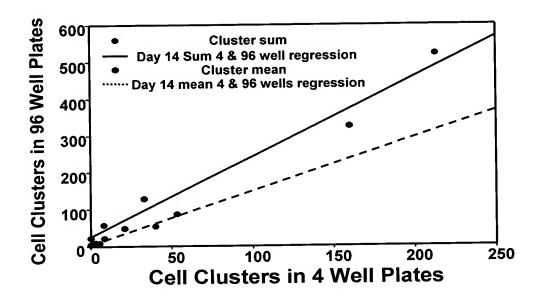


Fig. 5

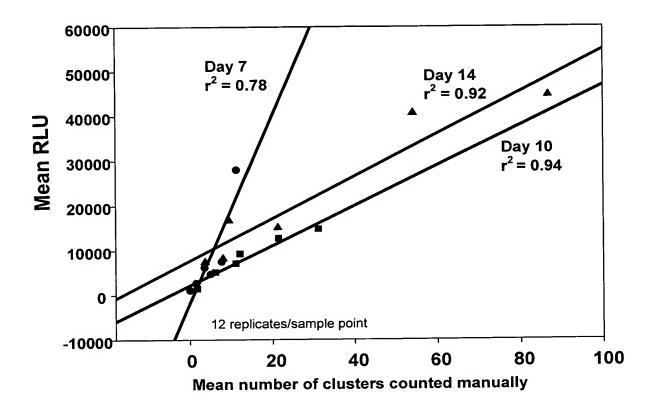
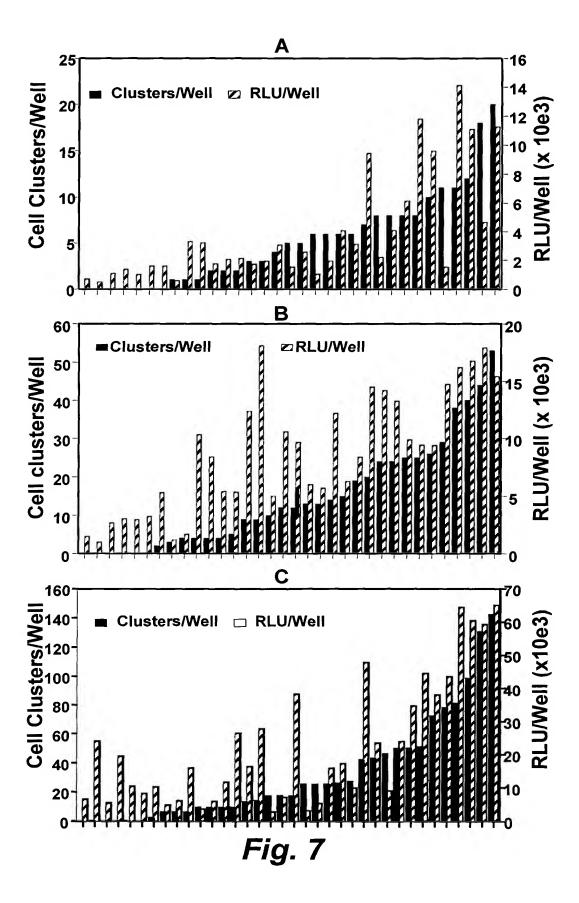


Fig. 6



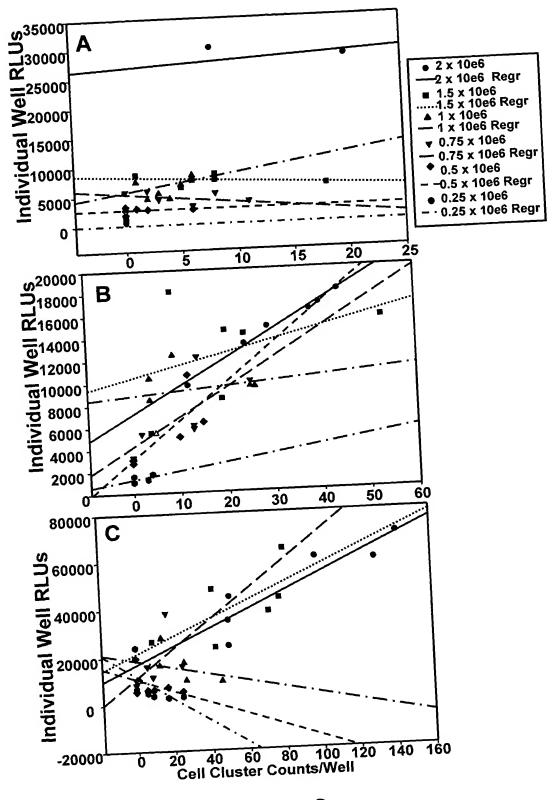


Fig. 8

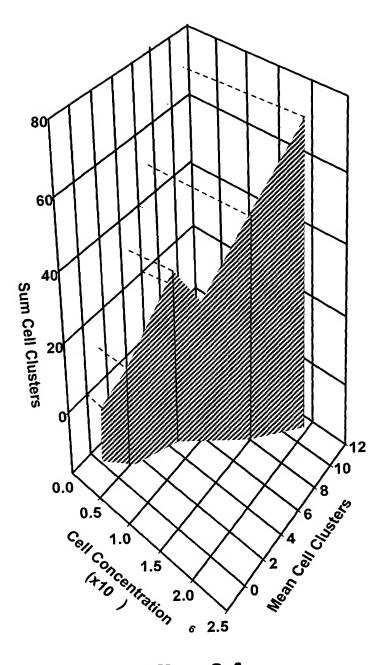


Fig. 9A

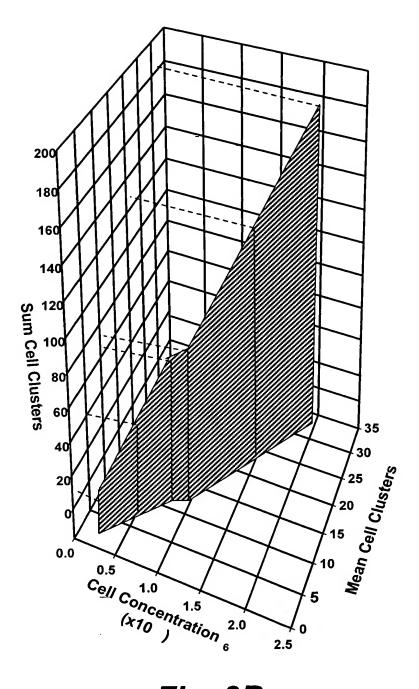
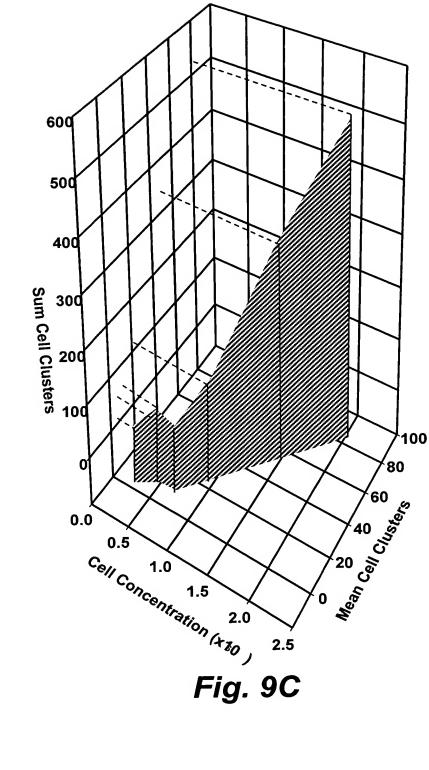


Fig. 9B



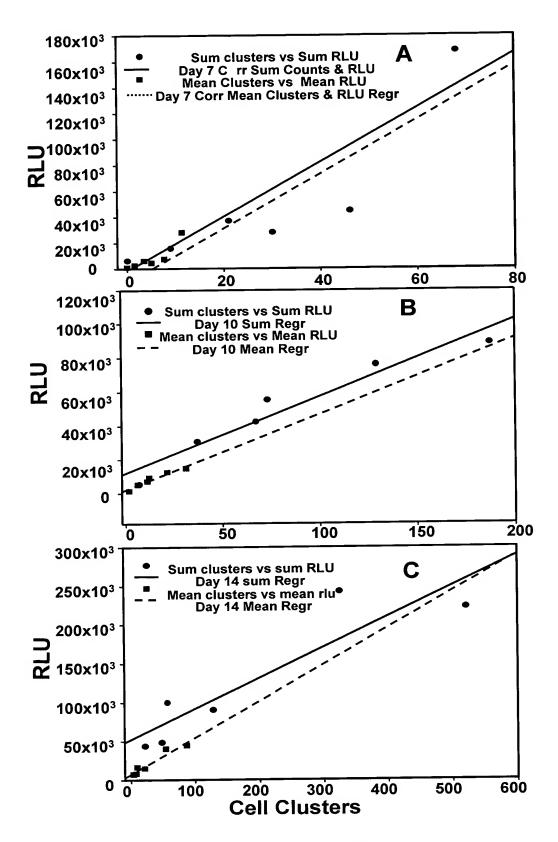


Fig. 10

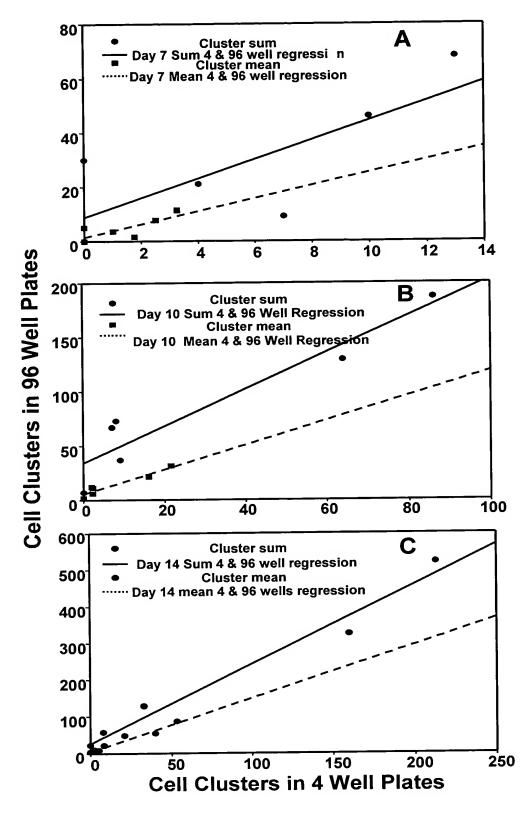


Fig. 11

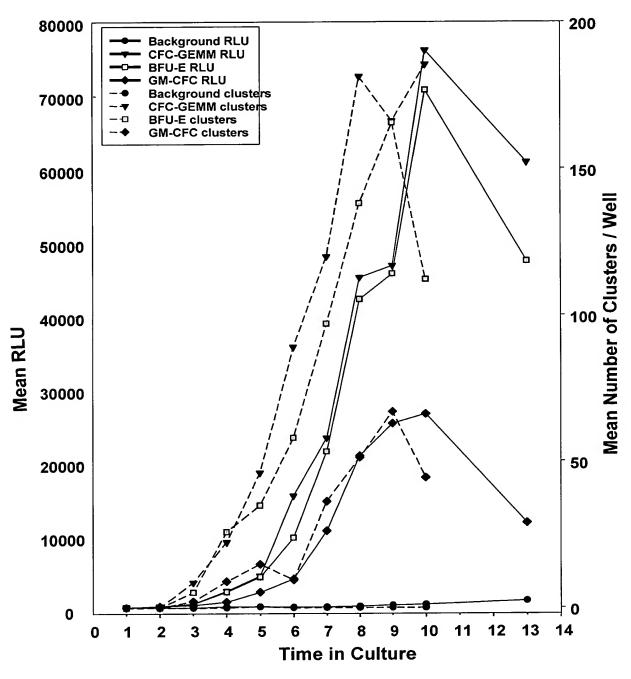


Fig. 12A

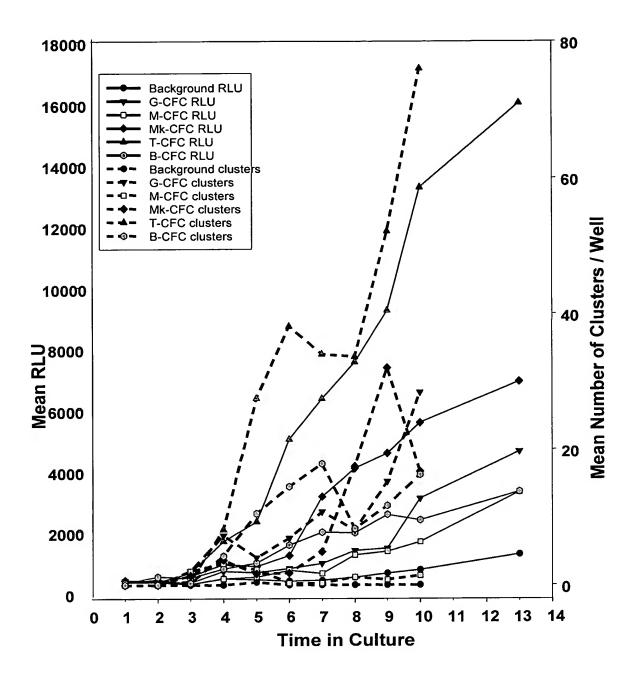


Fig. 12B

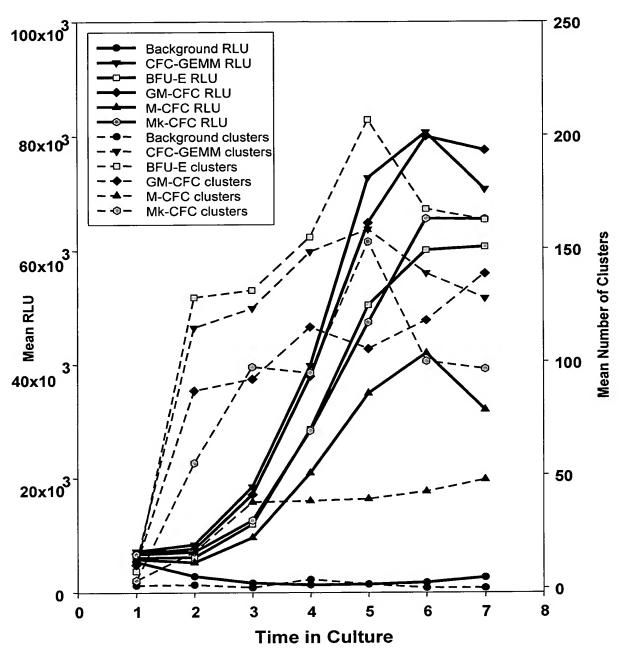


Fig. 13

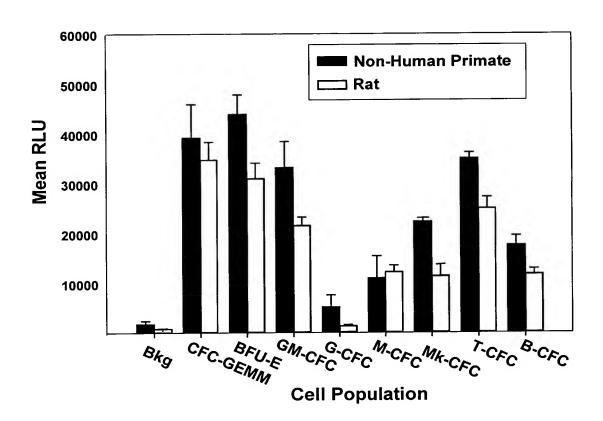


Fig. 14

A

30000
25000
20000
5000
10000
5000

Low [DOX] High [DOX]

Control Med [DOX]

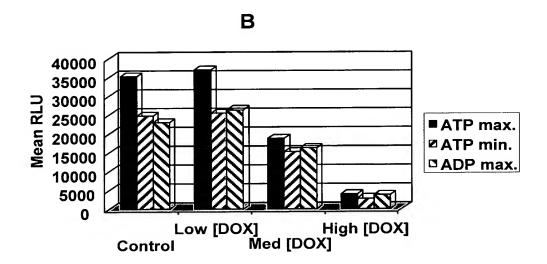
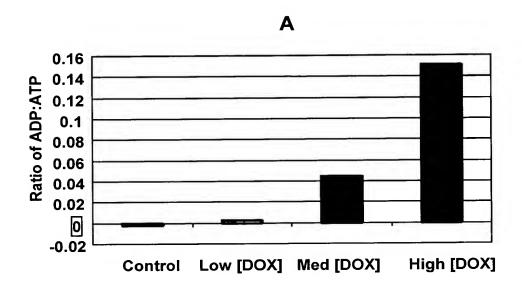


Fig. 15



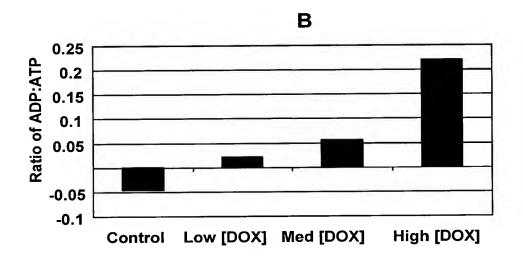


Fig. 16